


## 1. Objective

Seeding of a co-culture of Caco-2/HT29-MTX-E12 cells against extracellular matrix (ECM) gel in an OrganoPlate® 3-lane.



**Figure 1:** Schematic representation of an OrganoPlate® 3-lane tissue chip.

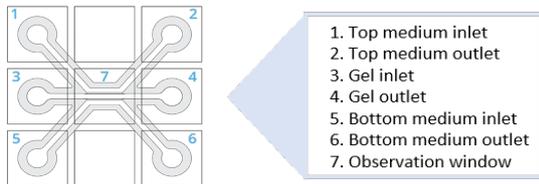

**Figure 2:** Illustration of a tubule of Caco-2 and HT29-MTX-E12 cells (top channel) grown against an ECM gel (middle channel) in an OrganoPlate® 3-lane tissue chip.

## 2. Background

Tubular structures, such as endothelial or epithelial barrier tissues, are established in the OrganoPlate® by growing cells against an ECM gel. Morphology and function of the tubule can be assessed by microscopy, a barrier integrity assay, or other functional assays. This protocol describes the culturing of a tubule of Caco-2 and HT29-MTX-E12 cells against ECM in the top lane of an OrganoPlate® 3-lane (see figure 1 and 2). The resulting tubular culture allows for access to apical and basal side of the barrier tissue.


## 3. Materials

- OrganoPlate® 3-lane (MIMETAS, 4004-400-B)
- OrganoFlow® S or L (MIMETAS, MI-OFPR-S or MI-OFPR-L)
- Human colon adenocarcinoma cell line Caco-2 (Sigma-Aldrich, 86010202)
- Human colon cell line HT29-MTX-E12 (Sigma-Aldrich, 12040401)
- Caco-2 medium components: EMEM (ATCC, 30-2003) + 10% FBS HI (ThermoFisher, 16140-071) + 1% Non-Essential Amino Acid (ThermoFisher, 11140050) + 1% Pen/Strep (Sigma, P4333)
- Collagen-I 5 mg/mL (AMSBio Cultrex® 3D collagen I rat tail, 5 mg/mL, 3447-020-01)
- 1 M HEPES (ThermoFisher, 15630-122, pH 7.2-7.5)
- 37 g/L NaHCO<sub>3</sub> (Sigma S5761-500G, dissolve in sterile MilliQ water, adjust pH to 9.5 using NaOH)
- Medium: 10 mL per OrganoPlate®
- Repeating pipette for gel loading and cell seeding, we recommend:
  - The Eppendorf® Multipipette® M4 with the Eppendorf® Biopur® 0.1 mL tip (VWR #613-2067) for dispensation of 2 µL, or
  - The Sartorius eLINE® electronic pipette (Sartorius, #735021) for accurate dispensation of volumes ranging from 0.2 to 10 µL. Use with corresponding Sartorius tips or with Eppendorf® ep Dualfilter tips (Eppendorf, 022491211 / 0030077512)
- HBSS (Sigma H6648)

- Multichannel pipette (1200 µL and 300 µl) and multichannel tips
- Crushed ice

## 4. Tubule seeding in the OrganoPlate®

A collagen-I ECM gel is loading in the gel inlet of the OrganoPlate® and fills the gel channel. After polymerization of the gel, a cell suspension is seeded in the top medium inlet and fills the top medium channel. After cell attachment, medium perfusion is started to aid the formation of a tubule (figure 3).

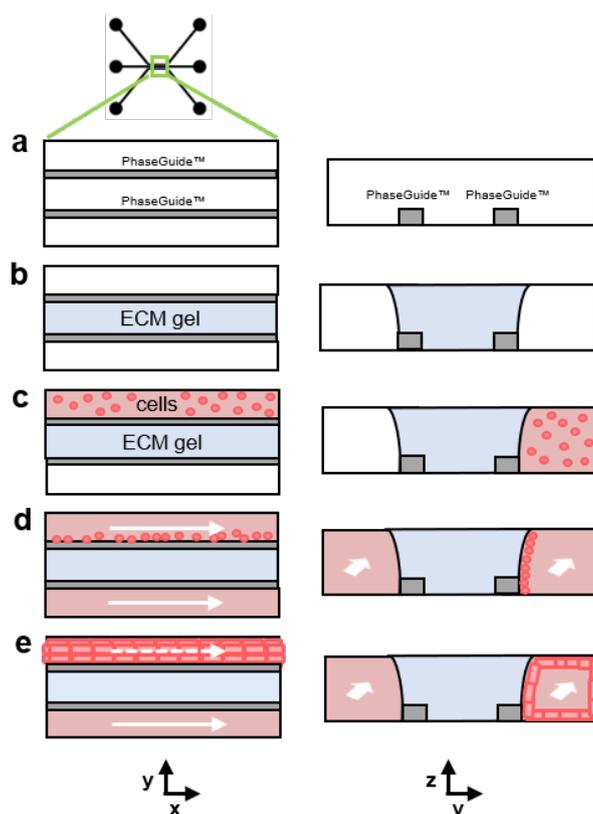

**Figure 3:** Schematic representation of tubule culture against ECM gel in the OrganoPlate® 3-lane

### Load ECM gel in the OrganoPlate®

*Note: avoid touching the bottom glass plate of the OrganoPlate®*

1. Take the OrganoPlate® from the packaging
2. Add 50 µL of HBSS to all wells in columns 2, 5, 8, 11, 14, 17, 20, and 23 using a multichannel repeating pipette. These columns contain the chips' observation windows
3. Prepare the required amount of ECM gel (e.g. 2 µL gel per chip + 40% extra)
  - a. Collagen-I 4 mg/mL preparation
    - i. Place an Eppendorf tube on ice
    - ii. The collagen-I 4 mg/mL gel is prepared by mixing 1 M HEPES, 37 g/L NaHCO<sub>3</sub>, and 5 mg/mL collagen-I in a 1:1:8 ratio. For example, to prepare 100 µL of gel:

- Place an Eppendorf tube on ice
  - Mix 10  $\mu\text{L}$  of 1 M HEPES with 10  $\mu\text{L}$  of 37 g/L  $\text{NaHCO}_3$
  - Add 80  $\mu\text{L}$  of collagen-I 5 mg/mL to the HEPES/ $\text{NaHCO}_3$  mixture
- iii. Prepare at least 100  $\mu\text{L}$  of total gel volume to ensure proper mixing of all components
  - iv. Mix well by pipetting the mixture up and down >20 times, while keeping it on ice
  - v. If bubbles are formed, quickly spin the tube down (~5 seconds)
  - vi. Use gel immediately after preparation (within 10 minutes)
4. Dispense the gel into the gel inlet (columns 1, 4, 7, 10, 13, 16, 19, 22; rows B, E, H, K, N) using the Eppendorf® Multipipette® M4 or the Sartorius eLINE electronic pipette.
    - a. Gently place your pipette tip on top of the hole in the bottom of the well and dispense the gel. Contact between the pipette tip and the hole is essential for gel loading. Correct positioning of the gel on top of hole allow capillary forces to pull the gel into the microfluidic gel channel (see figure 4).
    - b. The optimal loading volume depends on several factors, such as the viscosity of the gel and the temperature in the lab
    - c. Start by loading 2  $\mu\text{L}$  gel per gel inlet
    - d. In case of incomplete gel filling, increase the loading volume (i.e. to 2.3  $\mu\text{L}$ )
    - e. In case the gel overflows from the gel channel into the adjacent medium channel, reduce the loading volume (i.e. to 1.7  $\mu\text{L}$ )
  5. For examples of correct gel filling in the OrganoPlate® 3-lane, see figure 5.




Figure 4: Gel loading

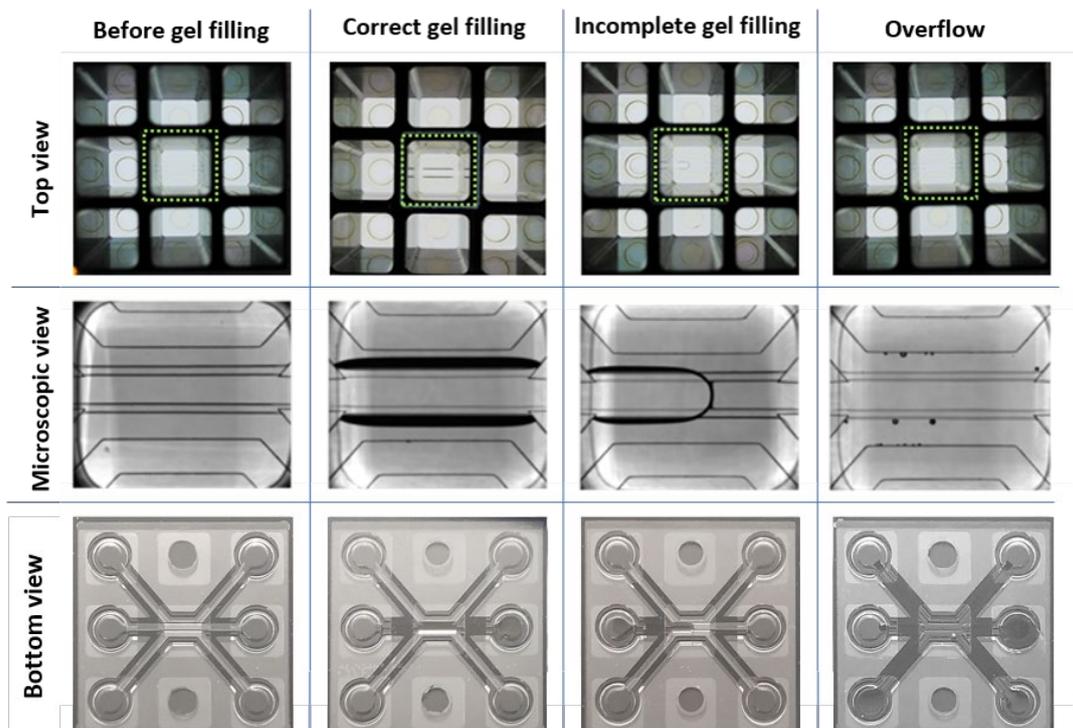


Figure 5: Overview of correct gel filling, incomplete gel filling, and overflow in the OrganoPlate® 3-lane.

Both the Eppendorf® Multipipette® M4 and the Sartorius eLINE electronic pipette can successfully be used to load gel in the OrganoPlate®. Table 1 shows an overview of each pipette’s advantages and disadvantages for gel loading.

**Table 1**

Pipette for gel loading	Advantage	Disadvantage
Eppendorf® Multipipette® M4	Allows user to load many chips in one go without having to reload the pipette tip*	Only allows whole-microliter volumes (1 µl, 2 µL, etc.), making it more difficult to correct incomplete gel filling or overflow
Sartorius eLINE® electronic pipette	Allows user to select the loading volume with 10 nL steps, such as 1.75 µL, 1.80 µL, 1.85 µL, etc.	Total volume of pipette is 10 µL, allowing user to load approximately 5 chips at a time before having to reload the pipette


\*We recommend loading a maximum of 20 chips at once before emptying and reloading the pipette tip with cold gel. This will avoid gelation of the gel while it is in the pipette tip.

6. Place the OrganoPlate® in a humidified incubator (i.e. 37°C, 5% CO<sub>2</sub>) for 15 minutes to allow polymerization of the collagen-I gel
7. Add 30 µL of HBSS to the gel inlet (columns 1, 4, 7, 10, 13, 16, 19, 22; rows B, E, H, K, N) to prevent the gel from drying out
  - a. For examples of dried out gel, see section 5. Trouble Shooting, figure 8.
8. Place the OrganoPlate® back in the incubator and proceed to cell seeding.
  - a. You can choose to proceed to cell seeding immediately or to wait until the next day. While cells generally form tubules with either option, Caco-2 cells show optimal results when seeded one day after gel loading.

## Seed Caco-2/HT29-MTX-E12 cells (ratio of 6:1) against the ECM gel


1. Harvest the Caco-2 and HT29-MTX-E12 cells according to their dissociation protocol
2. Before pelleting the cells by centrifugation, count the number of live cells in the cell suspension
3. Calculate the required number of cells for seeding in the OrganoPlate® and pellet them. For example:
  - a. Number of chips to seed: 40
  - b. Volume of cell solution to seed per chip: ~2 µL
  - c. Seeding density: 10,000 cells/µL
  - d. You need: 40 x 2 x 10,000 = 8.0\*10<sup>5</sup> cells (80 µL)
  - e. Prepare 25% extra: 1.0\*10<sup>6</sup> cells (100 µL)
  - f. Live cell count Caco-2 = 2.75\*10<sup>6</sup> cells/mL
  - g. Live cell count HT-29-MTX = 7.05\*10<sup>6</sup> cells/mL
  - h. Centrifuge them according to protocol
  - i. Prepare 1x concentration for both cell lines = 10.000 cells/µL
    - i. Caco-2 pellet from 1 mL solution (see f) + 275 µL media = 10.000 cells/µL
    - ii. HT-29-MTX pellet from 1 mL solution (see g) + 705 µL media = 10.000 cells/µL
  - j. Premix the Caco-2 and HT-29-MTX in 6:1 (v/v) (85.7 µL + 14.3 µL= 100 µL total) in a new Eppendorf tube

4. Remove HBSS from the gel inlets
5. Seed 2  $\mu\text{L}$  of cell suspension in the top medium inlet (columns 1, 4, 7, 10, 13, 16, 19, 22; rows A, D, G, J, M) using the same pipetting procedure as previously used for gel loading (see figure 3)
  - a. Regularly resuspend the cell suspension during seeding to ensure homogenous cell density.
  - b. In case you want to include cell-free controls, seed 2  $\mu\text{L}$  of medium without cells in the top medium inlet of these chips (instead of the cell suspension)
6. Add 50  $\mu\text{L}$  of medium to the top medium inlet (columns 1, 4, 7, 10, 13, 16, 19, 22; rows A, D, G, J, M)
7. Place the OrganoPlate® on its side in the MIMETAS plate stand for 3-4 hours in the incubator to allow the cells in the top channel to settle onto the ECM gel and attach (see figure 6).

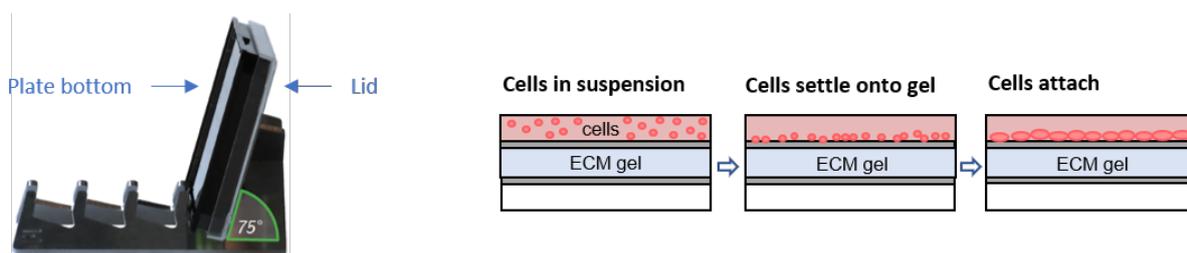


**Figure 6:** Incubate OrganoPlate® on the side to allow cells to attach to the ECM gel

8. After cells have attached, add 50  $\mu\text{L}$  of medium to the top medium outlet (columns 3, 6, 9, 12, 15, 18, 21, 24; rows A, D, G, J, M).
9. Add 50  $\mu\text{L}$  of medium to the bottom medium inlet (columns 1, 4, 7, 10, 13, 16, 19, 22; rows C, F, I, L, O)
  - a. Ensure that the medium has filled the channel completely
  - b. Ensure that no air bubbles are trapped on medium inlet and outlet. If bubbles are trapped, remove the bubbles gently with a pipette tip
10. Add 50  $\mu\text{L}$  of medium to the bottom medium outlet (columns 3, 6, 9, 12, 15, 18, 21, 24; rows C, F, I, L, O)
11. Place the plate on the OrganoFlow® in a humidified incubator to start cell culture (see figure 7)
  - a. An inclination of 7° and an interval of 8 minutes is optimal for most cultures

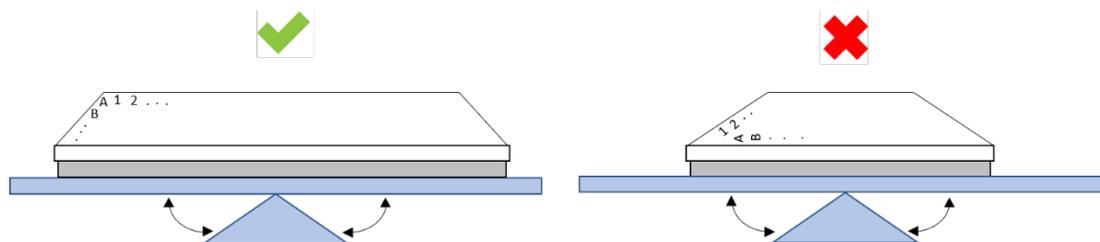

**Figure 7:** Place the OrganoPlate® on the OrganoFlow® in the correct orientation

12. Refresh medium every 2-3 days by aspirating and replacing the medium from medium inlets and outlets (50  $\mu\text{L}$  in each) using a repeating multichannel pipette
13. An example of a tubule culture against ECM in the OrganoPlate® 3-lane is shown in figure 8.

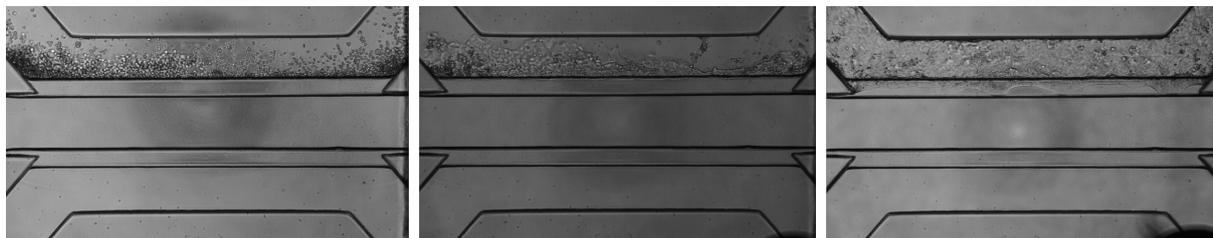


**Figure 8:** Caco-2/HT29 cells in the OrganoPlate 3-lane directly after seeding (left), after 1 day (middle) and after 4 days (right).

## 5. Troubleshooting

### ECM drying

In some cases, the ECM gel can dry out during the gel loading and polymerization process (figure 9). This generally happens when the gel loading process takes longer than expected and the gel in the chips that were loaded first has been incubated much longer than the gel in the chips that were loaded last. When loading goes smoothly, this problem doesn't occur. However, if loading takes longer than expected (> 10 min), check regularly under the microscope to see if the gel starts to dry out and if you observe that it is, quickly add HBSS to the gel inlet of those chips to prevent further drying.

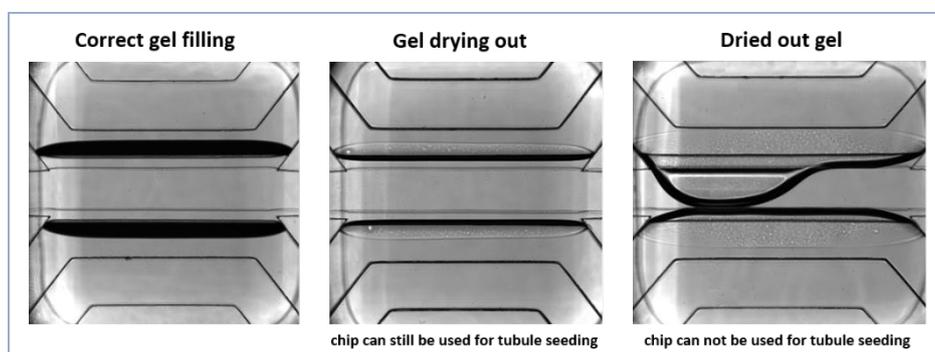


**Figure 9:** ECM gel drying out due to prolonged gel loading or polymerization

### Cell invasion

In case of undesired cell invasion into the gel, the use of MMP inhibitors is recommended (e.g. addition of 10 µM of MMP-I inhibitor GM6001 (Abcam, ab120845) to the culture medium).

Plate layout

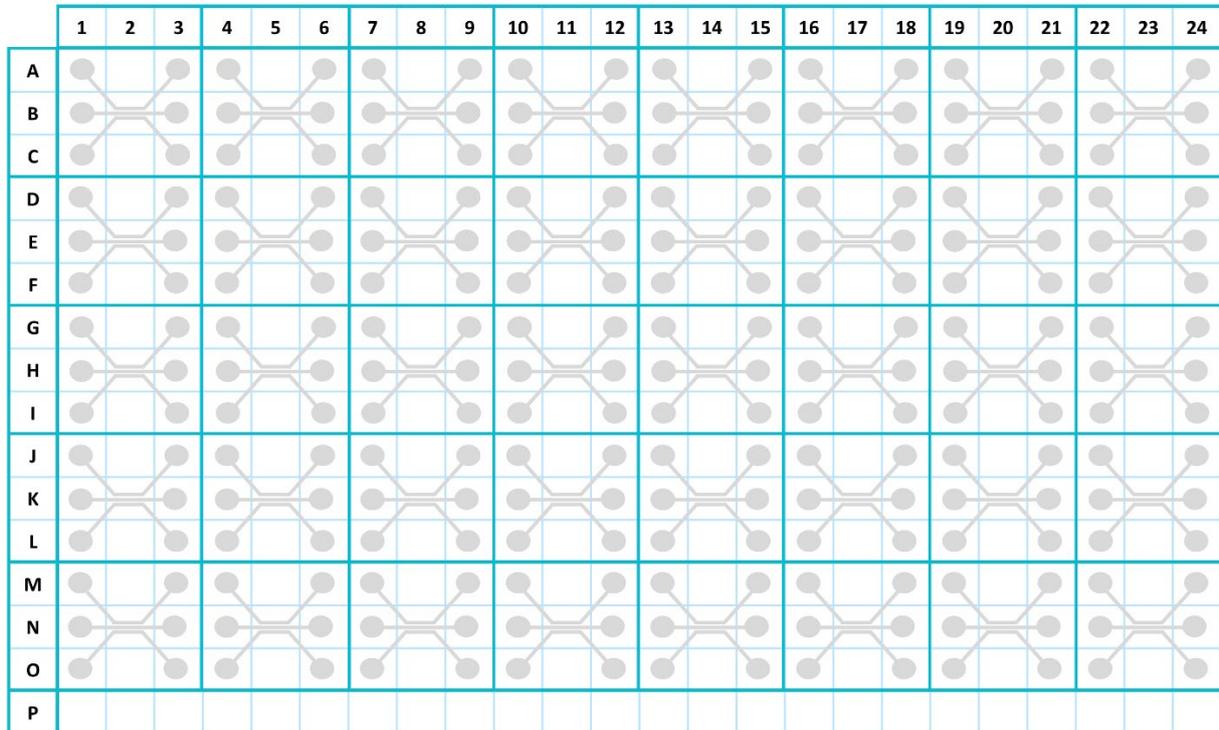

## MIMETAS product list

Cat. No.	Product Name
MI-AR-CC-01	OrganoReady® Caco-2
9605-400-B	OrganoPlate® 2-lane
4004-400-B	OrganoPlate® 3-lane 40
6405-400-B	OrganoPlate® 3-lane 64
6401-400-B	OrganoPlate® Graft
MI-OFPR-S	OrganoFlow® S
MI-OFPR-L	OrganoFlow® L
MI-OT-1	OrganoTEER®

## Contact information

For questions, please contact us through the e-mail addresses stated below

**Purchasing:** [order@mimetas.com](mailto:order@mimetas.com)

**Customer service:** [info@mimetas.com](mailto:info@mimetas.com)

**Technical support:** [support@mimetas.com](mailto:support@mimetas.com)

### MIMETAS Europe

J.H. Oortweg 19  
2333 CH, Leiden  
The Netherlands  
Phone: +31 (0)85 888 3161

### MIMETAS USA

704 Quince Orchard Road  
Suite 260, MD 20878  
Gaithersburg, USA  
+1 (833) 646-3827

### MIMETAS Japan

4F Tekko Building,  
1-8-2 Marunouchi, Chiyoda-Ku  
Tokyo, 100-0005, Japan  
+81 3-6870-7235

This protocol is provided 'as is' and without any warranties, express or implied, including any warranty of merchantability or fitness for a particular purpose or assured results, or that the use of the protocol will not infringe any patent, copyright, trademark, or other proprietary rights. This protocol cannot be used for diagnostic purposes or be resold. The use of this protocol is subject to Mimetas' General Terms and Conditions of Delivery, Purchase and Use.

MIMETAS®, OrganoPlate®, OrganoFlow®, OrganoReady®, and OrganoTEER® are registered trademarks of MIMETAS BV. Cultrex® is a registered trademark of Trevigen, Inc. Eppendorf®, Multipette®, and Biopur® are registered trademarks of Eppendorf AG, Germany. eLINE® is a registered trademark of Sartorius Biohit Liquid Handling Oy.